

unipower

Veterinary Equipment



Replacement Batteries



WARRANTY AND GENERAL INFORMATION

Warranty:

Unipower warrants all equipment manufactured by it to be free from defects in material and workmanship for a period of twelve months from date of sale. All statements, technical information and recommendations contained herein are based on tests Unipower believes to be reliable, the accuracy or completeness thereof is not guaranteed.

Notwithstanding any special extended or limited warranty published by Unipower, Unipower's sole remedy will be to repair or replace any part of the equipment determined by Unipower to be defective. **This warranty is exclusive, and is in lieu of any other warranties, express or implied, including but not limited to, WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE.** In no event will Unipower be liable for indirect, incidental, special or consequential damages, whether due to breach of contract, breach of warranty, the negligence of Unipower, or otherwise.

Unipower makes no warranty in connection with accessories, equipment, materials or components sold but not manufactured by Unipower. These items are subject to the warranty, if any, of their manufacturer. Unipower will provide reasonable assistance in making any claim for breach of the original manufacturer warranty.

No statement or recommendation not contained herein will have any force or effect unless in an agreement signed by representatives of Unipower.

Special Extended and Limited Warranties:

<u>Product Type</u>	<u>Description</u>
Lead Acid Batteries	16 Months Full
Medical NiCad Packs	16 Months Full
Hawker Lead Acid	12 Months Full
Cables and Harnesses	90 Days
Non-Rechargeable	Will be free from defects and perform at rated capacity at time of delivery.

Terms:

Net 30 days from date of invoice.

Pricing:

All orders are shipped on the basis of prices prevailing at the time the order is accepted. Prices are subject to change without notice.

Delivery and Transportation:

Unless agreed to by Unipower at time of order acceptance, all orders are FOB Unipower, prepay and add.

Credits and Exchange:

A Return Goods Authorization (RGA) number must accompany all products returned for a credit or exchange. Please contact your distributor or Unipower for an RGA prior to returning any products. Items returned due to customer error are subject to a 20% re-stocking fee.

Battery Disposal:

A Recycle Authorization (R) number must accompany all products returned for disposal. Please contact your distributor or Unipower for an R number prior to returning any products for disposal.

Shortages, Errors, and Shipping Damage:

All claims for shortages, errors, and shipping damage must be made within 7 business days of receipt of order to your distributor or Unipower.

MODEL	OEM P/N	PART #	VOLTS	AMPS	CHEMISTRY	NOTES
<u>ABBOTT MEDICAL ELECTRONICS</u>						
DH 5 Monitor/Defibrillator		B10148	24.0V	1.6Ah	NiCad	
Life Care 5000, 5500, 6000 Infusion Pump		B10796	8.0V	2.8Ah	Lead Acid	
Plum Infusion Pump		B10796	8.0V	2.8Ah	Lead Acid	
<u>BAXTER HEALTHCARE</u>						
AS40, AS41 Infusion Pump		B10669	6.0V	1.0Ah	NiCad	
AS50A Infusion Pump		B11056	6.0V	2.15Ah	NiMH	
Colleague Infusion Pump		B00355	12.0V	2.0Ah	Lead Acid	
Colleague Infusion Pump-Memory		B11192	7.2V	2.1Ah	Li/SOCl ₂	
Flo-Gard 6200 Infusion Pump		B10326	4.0V	6.0Ah	Lead Acid	2/Unit
Flo-Gard 6201 Infusion Pump		B00355	12.0V	2.0Ah	Lead Acid	
Flo-Gard 6201, 6301-Memory		B10920	3.0V	1.1Ah	Li/MnO ₂	
Flo-Gard 6300, 6301 Infusion Pump		B00330	12.0V	3.2Ah	Lead Acid	
<u>BURDICK INC</u>						
E500, E600 EKG Monitor		B10378	9.6V	0.6Ah	NiCad	
E500, E600, E350I EKG Machine-Memory Back-up		B10712	3.0V	1.2Ah	Li/MnO ₂	
<u>CRITIKON INC</u>						
Compact TS Monitor		B00932	12.0V	2.3Ah	Lead Acid	
8100, 8100T, 8110 Dinamap Monitor		B10333	12.0V	2.8Ah	Lead Acid	
<u>DATASCOPE CORP</u>						
M/D4 Monitor/Defibrillator		B10526	12.0V	2.5Ah	NiCad	Rebuild
Passport, Passport 2, Passport 2 LT, Passport XG Monitor		B00932	12.0V	2.3Ah	Lead Acid	2/Unit
Passport, Passport 2 Monitor-Memory		B01811	3.0V	0.19Ah	Li/MnO ₂	
<u>DATEX-OHMEDA</u>						
Modulus 2 Plus		B00914	6.0V	12.0Ah	Lead Acid	2/Unit
5250 RGM Monitor		B01813	3.0V	0.54Ah	Li/MnO ₂	
7000 Ventilator		B00116	7.2V	0.15Ah	NiMH	
7800 Ventilator		B10788	4.8V	1.6Ah	NiCad	
7900 Ventilator	1503-3045-000 Rev 01	B11102	12.0V	2.6Ah	Lead Acid	
<u>DETECTO SCALE</u>						
IB400 Digital Scale		B10654	12.0V	1.6Ah	NiCad	
6475, 6800, 8430B Digital Scale		B10654	12.0V	1.6Ah	NiCad	
<u>DRAEGER MEDICAL INC</u>						
Narkomed 2A Anesthesia Machine		B10863	12.0V	7.5Ah	Lead Acid	
Narkomed 2B Anesthesia Machine		B00924	12.0V	7.2Ah	Lead Acid	
Narkomed 2C Anesthesia Machine		B00928-1	12.0V	18.0Ah	Lead Acid	
<u>HILL-ROM CO INC</u>						
Century CC Scale		B00938	6.0V	2.8Ah	Lead Acid	
<u>INVIVO RESEARCH INC</u>						
4500 Scout Mini O ₂ Monitor		B10795	4.8V	1.6Ah	NiCad	
<u>MARQUETTE ELECTRONICS</u>						
Mac PC, Mac 6 ECG Recorder		B10412	19.2V	1.6Ah	NiCad	
46 Monitor/Defibrillator		B10148	24.0V	1.6Ah	NiCad	
<u>MILES INC</u>						
VIP 2000 Tissue Sampler		B10758	3.0V	0.65Ah	Li/(CF) _n	
1000, 3000 Tissue Processor		B10762	3.0V	0.65Ah	Li/(CF) _n	
<u>NELLCOR PURITAN BENNETT INC</u>						
N-180, N-185 Pulse Oximeter		B00932	12.0V	2.3Ah	Lead Acid	
N-1000 Multi Function Monitor		B10519	6.0V	2.8/4.5Ah	Lead Acid	
<u>NOVAMETRIX MEDICAL SYSTEMS</u>						
610, 615 Tidal Wave Handheld Capnograph		B11144	7.2V	3.5Ah	NiMH	
710, 715 Tidal Wave Handheld Capnograph	400043	B11195	7.2V	3.8Ah	NiMH	
<u>OEC-DIASONICS INC</u>						
Uroview 2000		B10791	384.0V	12.0Ah	Lead Acid	
Uroview 2500		B10891	420.0V	12.0Ah	Lead Acid	

MODEL	OEM P/N	PART #	VOLTS	AMPS	CHEMISTRY	NOTES
<u>OLYMPUS AMERICA INC</u>						
CLE F10 Light Source		B10756	3.0V	Lith	Li/MnO ₂	
CLV10 Light Source		B10672	3.0V	Lith	Li/MnO ₂	
CLV-U20, CLV-U40 Light Source	GU142400	B11263	3.6V	2.4Ah	Li/SOCl ₂	
CVI Light Source		B10672	3.0V	Lith	Li/MnO ₂	
CV100	DP034100	B11364	3.6V	0.85Ah	Li/SOCl ₂	
CV100	DP034200	B10672	3.0V	Lith	Li/MnO ₂	
CV100	GU142400	B11263	3.6V	2.4Ah	Li/SOCl ₂	
CV200	GU124400	B11264	3.6V	2.4Ah	Li/SOCl ₂	
<u>PHILIPS MEDICAL SYSTEMS CARDIAC & MONITORING</u>						
M1722A/B, M1723A/B, M1724XE Codemaster	M1758A	B10782	12.0V	5.0Ah	Lead Acid	
M43100A, M43110A, M43130 Monitor/Defibrillator		B10205	12.0V	2.5Ah	Lead Acid	
M78353B Patient Monitor		B10231	24.0V	2.2Ah	NiCad	
M78534A Monitor		B10279	7.2V	0.7Ah	NiCad	Insert
M78554A Data Management Module		B10279	7.2V	0.7Ah	NiCad	Insert
M78560A Central Monitor		B10932	3.6V	0.7Ah	NiCad	
M78560A Monitor-Back-up Board		B10279	7.2V	0.7Ah	NiCad	Insert
<u>PHYSIO-CONTROL</u>						
LifePak 5 Standard Charge		B10027	12.0V	1.6Ah	NiCad	
LifePak 9 Monitor/Defibrillator		B10430	16.0V	2.8Ah	Lead Acid	
LifePak 9, 9P Upgrade	803704-03	B11053	16.0V	2.5Ah	Lead Acid	
LifePak 10 Monitor/Defibrillator		B10473	12.0V	1.3Ah	NiCad	3/Unit
LifePak 11 Monitor/Defibrillator		B10473	12.0V	1.3Ah	NiCad	
LifePak 12 Monitor/Defibrillator						
OEM BATTERY	11141-000028	B11460	12.0V	2.5Ah	Lead Acid	
OEM BATTERY	11141-000026	B11461	12.0V	2.4Ah	NiCad	
OEM BATTERY	11141-000027	B11462	12.0V	1.7Ah	NiCad	
LifePak 12 without fuel gauge		B11329	12.0V	2.4Ah	NiCad	
LifePak 12, FPII without fuel gauge		B11170	12.0V	1.9Ah	NiCad	
LifePak 250		B10473	12.0V	1.3Ah	NiCad	
<u>PULMONETICS</u>						
LTV Universal Power Supply	14546-001	B00340-1	12.0V	80W	Lead Acid	
LTV Ventilator 900, 950, 1000		B11157	12.0V	5.0Ah	Lead Acid	
<u>PURITAN BENNETT CORP</u>						
PB2801	20837	B10930	12.0V	4.5Ah	Lead Acid	
7200 Ventilator		B01002	2.0V	5.0Ah	Lead Acid	2/Unit
<u>SABRATEK CORP</u>						
3030 Infusion Pump		B00330	12.0V	3.2Ah	Lead Acid	
3030 Clock Battery		B11188	3.0V	0.165Ah	Li/(CF) _n	
<u>SECA CORP</u>						
727 Electronic Scale (7.2V Version)		B11121	7.2V	0.7Ah	NiCad	
727 Electronic Scale (9.6V Version)		B10765	9.6V	0.7Ah	NiCad	
728 Electronic Scale	68-22-12721	B11269	7.2V	1.6Ah	NiMH	
<u>SIEMEN'S MEDICAL SYSTEMS</u>						
Servo 300 Ventilator		B00317	12.0V	2.3Ah	Lead Acid	2/Unit
Servo 300-Memory		B11080	3.6V	2.5Ah	Li/SO ₂ Cl ₂	
900C		B11080	3.6V	1.9Ah	Li/SO ₂ Cl ₂	
<u>SMITHS MEDICAL MD INC</u>						
CADD TPN 5700 Infusion Pump	21-2357	B10729	12.0V	1.2Ah	NiCad	
CADD TPN 5700 Infusion Pump	21-3802	B10966	12.0V	1.8Ah	NiMH	
<u>SPACELABS MEDICAL INC</u>						
4045 Monitor/Defibrillator		B10148	24.0V	1.6Ah	NiCad	
<u>VIASYS HEALTHCARE INC</u>						
4400 Portable Oximeter 9545, 9579		B10816	4.8V	0.7Ah	NiCad	
<u>ZOLL MEDICAL CORP</u>						
PD 900, 1200 Pacemaker Monitor/Defibrillator	9145-0003	B10544	12.0V	2.5Ah	Lead Acid	
PD 1400, 1600, 2000 Monitor/Defibrillator		B11099	10.0V	2.5Ah	Lead Acid	

For your convenience, Unipower offers our catalogs in multiple formats. You may download a copy from our website www.unipower.com, or have one emailed to you. Email your requests to: unipower@unipower.com.

If you prefer a catalog by mail, simply request one by calling (800) 542-6998.



Biomedical: Power for Hospital, Surgical, and Emergency Medical Equipment.



Cables & Lead Wires: ECG Monitoring Cables and Lead Wires.



Communications: Two Way Radios.



Sealed Lead-Acid: Reliable Power for Electronic Equipment.



UPS: Back-Up Power for Your Technology Equipment.



Veterinary: Specialty Batteries for Animal Diagnostic and Surgical Devices.



Portable X-Ray: Power for Imaging Equipment.

In addition to the above listed catalogs, please call to inquire about our batteries from the following categories:



Alarm / Security.



Emergency Lighting.



Test Equipment.


We Also Offer Replacement Batteries for...



- UPS Systems
- Emergency Lighting
- Alarm and Security Systems

And a Full Line of ...

- ECG Monitoring Cables
- Leadwires
- Dual Socket Cables and Leadwires

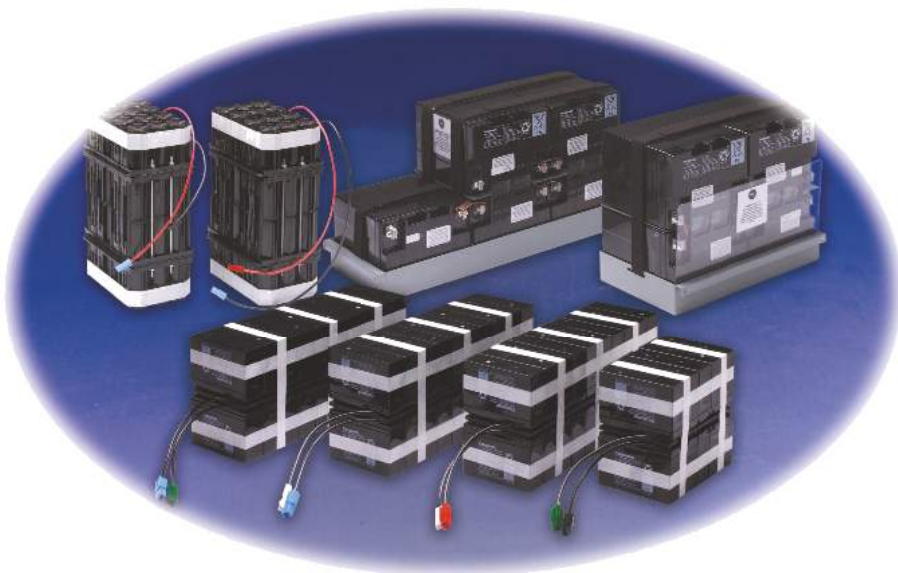

Plus Replacement Batteries and Kits for...

- Portable X Ray Machines
- C-Arms